

MANUAL TO OBTAIN IFUS FROM THE WEB



sales@operon.es

www.operon.es

INDEX

1 OPERATION INSTRUCTIONS.....3

1.1 INTRODUCTION.....3

1.2 HOW TO ACCESS TO THE WEB WHERE THE IFUs ARE LOCATED.....3

1.3 HOW TO DOWNLOAD THE IFUS FROM THE WEB.....3

1.4 HOW TO OBTAIN A PAPER COPY OF THE IFUS.....6

1 OPERATION INSTRUCTIONS

1.1 INTRODUCTION

The Instructions of Use of the Products designed to be used for Professionals are only available through a specific webpage, they are not provided inside the kit.

The information necessary to download the correct version of the instructions for use is indicated on the external label (for Immunochromatography products) or on the internal label (for Molecular Biology products), attached to the inner flap of the box.

A summary of the Procedure of the kit will also be available inside the kit.

1.2 HOW TO ACCESS TO THE WEB WHERE THE IFUS ARE LOCATED

The webpages where the IFU can be downloaded are:

1. <https://ifus.operon.es/operon>
2. Through Operon's website, main menu, IFU section.


<http://www.operon.es/>

1.3 HOW TO DOWNLOAD THE IFUS FROM THE WEB

1. The main page will have this appearance:



2. Select the desired language (English or Spanish) of the webpage.

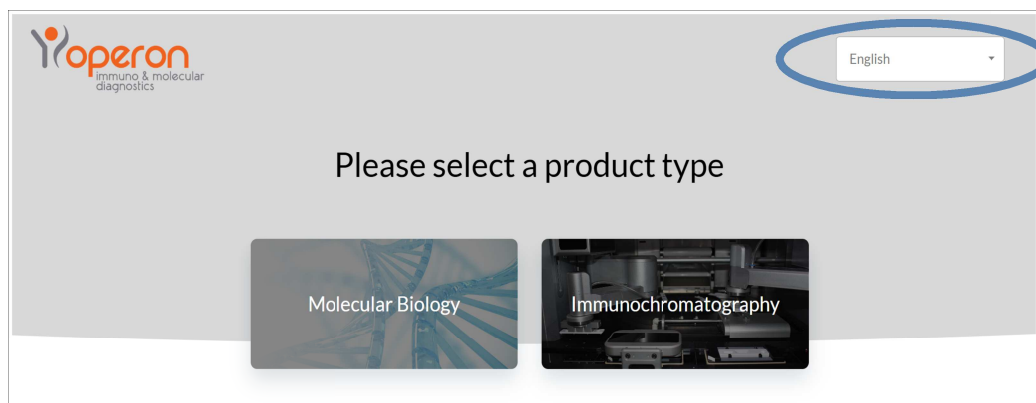

3. Select the type of product of interest: Immunochromatography or Molecular Biology.
4. Enter the Name or Reference data in the menu, these data appear on the product labeling. For immunochromatography products on the external label and for molecular biology products on the internal label of the box, attached to the inner flap of the box. In the case of Reference, please note that you must enter only the first four digits (including the point). Example X.XXX

Example of labeling products Immunochromatography

KIT LABEL / ETIQUETA KIT

NAME / NOMBRE ← **Simple Rota-Adeno-Noro**

LOT BH25-B125.25 REF 9.050 020.15.000 2026.12

REFERENCE / REFERENCIA

REFAG RAN LOT BH25-B125 2026.12

CTL 06 LOT 25 2026.12

2°C 30°C 200 test CE 0197 IVD B Rev. 01

Simple Rota-Adeno-Noro
Resusita, Adenovirus, Norovirus GI/GII

DOCUMENT NUMBER / N° DOCUMENTO ← IFU-0905113 Rev. 05

VERSION / VERSIÓN

Control Rota-Adeno-Noro
Control Rotavirus, Adenovirus, Norovirus GI/GII

OPERON, S.A.
Carretera del Plano, 19. 50410.
Caspe de Trueno, Zaragoza, Spain.
MADE IN SPAIN

016042957790731
(17)051291
(10)BH25-B125.25

CONTROLS LABEL / ETIQUETA CONTROLES

NAME / NOMBRE ← **Rota-Adeno-Noro**

Control Rotavirus, Adenovirus, Norovirus GI/GII

REF 9.050 011.12.000 CONTROL 2027.03

LOT BH25B125

1 swab CE 0197 Rev. 03

REFERENCE / REFERENCIA

Rota-Adeno-Noro
Control Rotavirus, Adenovirus, Norovirus GI/GII

OPERON, S.A.
Carretera del Plano, 19. 50410.
Caspe de Trueno, Zaragoza, Spain.
MADE IN SPAIN

016042957790731
(17)051291
(10)BH25-B125.25

DOCUMENT NUMBER / N° DOCUMENTO ← IFU-0905113 Rev. 05

VERSION / VERSIÓN

Example of labeling products molecular biology

KIT LABEL / ETIQUETA KIT

NAME / NOMBRE ← **HLA B5701 Strip**

REF 3.155 048.53.000 LOT B5701 01.2014 2013.03

(ifus.operon.es) IFU-09051024 Rev. 06

REFERENCE / REFERENCIA **LOT** **VERSION / VERSIÓN**

		B5701.05.2015	2015.06	
STRIPS	Strips			24 x 2
SOL DN	Denaturing solution			1 ml
BUF HYB	Hybridization buffer			125 ml
BUF WASH 1	Washing buffer 1	17	2015.03	250 ml
CONJ HRP	Conjugate	25	2015.07	125 ml
BUF WASH 2	Washing buffer 2	33	2015.25	350 ml
SUBS TMB	Chromogen substrate	30	2015.11	65 ml
PCR MIX	PCR Mix	05	2015.05	3 x 1.40 ml
TAQ	TAQ	09	2015.11	0.120 ml
PRIMERS	Primers A B5701	12	2015.07	0.275 ml
	Primers B B5701	22	2015.10	0.275 ml

DOCUMENT NUMBER / N° DOCUMENTO

OPERON, S.A. Rev. 04 ! NO TIRAR LA CAJA EXTERIOR / DO NOT DISCARD THE EXTERNAL BOX

5. Once the Name or Reference is selected, press the “Search” button to obtain the list of all the documents available for this reference or name,

Name

Type here...

Reference

9.050

Search

Name


Rota-Adeno-Noro

Reference

Type here...

Search

6. Select the number of the document (IFU-0905XXXX) and the version (Rev. XX) of the document that is indicated in the label of the product (the external one for immunochromatographic products and the internal one for molecular diagnostic products, attached to the inner flap of the box).



NOTE: the version of the instruction is dependent on the lot. The version of the instruction might not be the latest one, but it is the one that has to be used.

Detalle del producto:

NOMBRE: Rota-Adeno-Noro

REFERENCIA: 9.050.XXX.YYY.ZZZ

ATENCIÓN: Seleccione el número de documento (IFU-0905XXXX) y la versión (Rev. XX) de las instrucciones de uso que esté indicada en la etiqueta del producto. Tenga en cuenta que la versión depende del lote, lo que implica que quizá la versión no sea la última, pero es la que debe utilizarse.

IFU-0905XXXX Rev. XX

Atención: Para abrir archivos PDF, se necesita Adobe Acrobat Reader. [Haga clic aquí](#) para ir al sitio web de Adobe y descargar una copia gratuita.

IFU:

PDF

IFU-0905151.Rev04

IFU-0905151-ROTA-ADENO-NORO-04

Mostrar idiomas disponibles

PDF

IFU-0905151.Rev05

IFU-0905151-ROTA-ADENO-NORO-05

Mostrar idiomas disponibles

PDF

IFU-0905171.Rev03

IFU-0905171-CPS-ROTA-ADENO-NORO

Mostrar idiomas disponibles

7. Click on “Show available languages” and the available languages will be displayed.

IFU:

PDF

IFU-0905151.Rev04

IFU-0905151-ROTA-ADENO-NORO-04

Mostrar idiomas disponibles

PDF

IFU-0905151.Rev05

IFU-0905151-ROTA-ADENO-NORO-05

Ocultar idiomas disponibles

VERSION MÁS RECIENTE

Česky/cs - Czech

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

English/en - English

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Français/fr - French

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Polski/pl - Polish

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Ελληνικά/el - Greek

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Deutsch/de - German

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Español/es - Spanish

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05


Italiano/it - Italian

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

Português/pt - Portuguese

IFU-0905151-ROTA-ADENO-NORO-05 - 17/3/2025 - 05

8. Select the required language by pressing the red arrow located on the right of the language. A download confirmation message will appear with the relevant information: press "confirm" to start the downloading process.

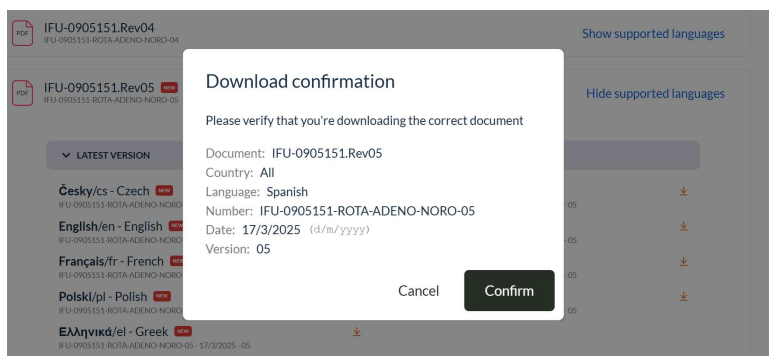

9. Search the document for the required language with the help of the index.

1.4 HOW TO OBTAIN A PAPER COPY OF THE IFUS

The user can ask for a paper copy of the IFU

1. Directly to Operon (sales@operon.es)
2. By calling the following international free telephone number: +800 135 79 135. Depending on the country, other free telephones can be used:
 - Canada: 1 855 805 85 39
 - Lithuania: 880 030728
 - US: 1 855 236 09 10
 - Liechtenstein*: +31 20 796 56 92
 - Chile: 800 914 248
 - Mexico: +52 800 953 07 45
 - Turkey: 00 800 142 064 866
 - Vietnam: 122 80297
 - Rest of the world*: +31 20 794 7071

* Pay number

IT-020103

OPERON, S.A.
Camino del Plano 19
50410 Cuarte de Huerva
Zaragoza - ESPAÑA
Tel. + 34 976503597
Fax: + 34 976503531